


HORIZON PRO 639 LSO PATIENT APPLICATION


PRODUCT INFORMATION

HORIZON PRO 639 LSO

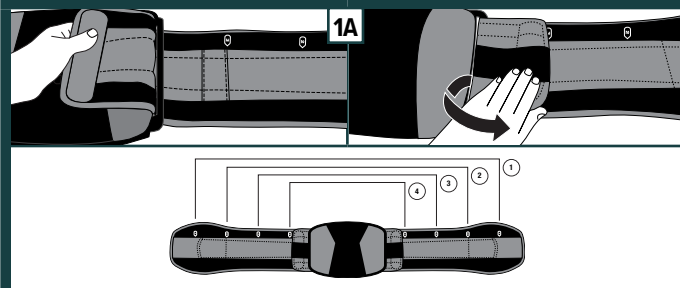



1. SIZE ADJUSTMENT

1A. To change the size of the Horizon, peel up the inside end of the side panel on each side. Adjust to proper fit and reattach.

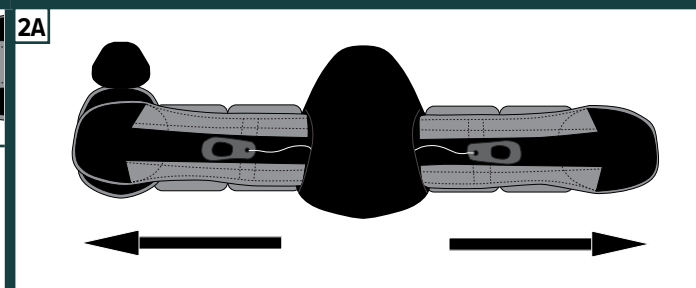


2. PREPARATION



2A. Place the pull tabs 2 inches (5 cm) from the plastic in the back of the brace. Pull the ends of the brace away from each other ensuring that it is fully extended.

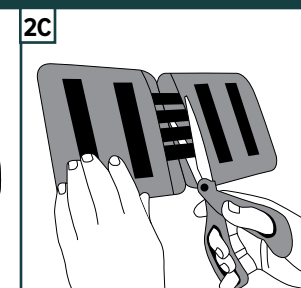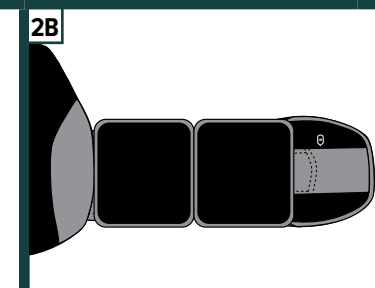


2B. Confirm that the lateral panels extend from posterior to anterior panels.
2C. For smaller patients, lateral panels may need to be trimmed down to one panel. Once trimmed, tuck exposed plastic end into the sleeve.

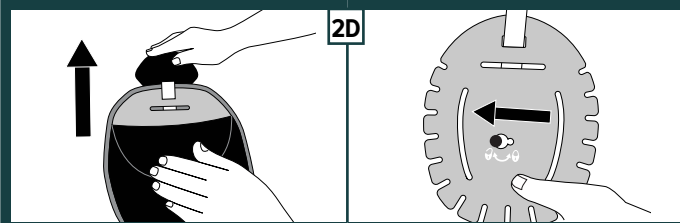

D. For shorter patients, the top extension panel may be taken off by removing the plastic anterior panel from the sleeve. Slide the aluminum bar to unlock. Once removed, reinsert the plastic anterior panel back into the sleeve

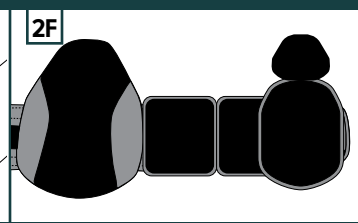
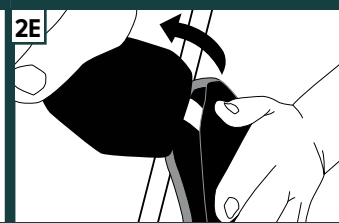


E. For patients requiring the top extension panel, the aluminum bar may be bent to accommodate patient anatomy.
F. Align and attach left side panel to rigid anterior panel to accommodate patient anatomy.


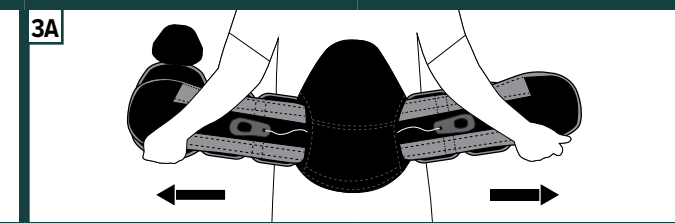


3. APPLICATION

A. Apply the fully extended brace making sure the back panel is centered and low on the back. Apply the brace tightly around the abdomen, the right side overlapping the left.

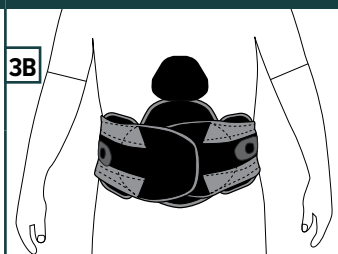
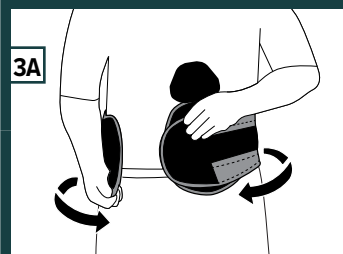


B. When applied properly, both the upper and lower edge of the brace should be snug. If there is any gap, reapply the brace and angle the ends to insure a snug fit at both the upper and lower edge.
NOTE: For certain patients, the ends must be steeply angled.

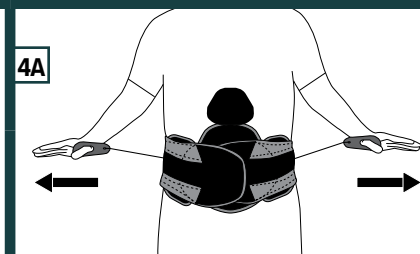

4. TIGHTENING

A. Slip your thumbs through the holes in the pull tabs. Pull away from your body.
B. The left pull tab controls lower compression and the right pull tab controls the upper compression. Adjust the compression as needed.
C. When tightened, secure the pull tabs to the hook-and-loop in front of the brace.

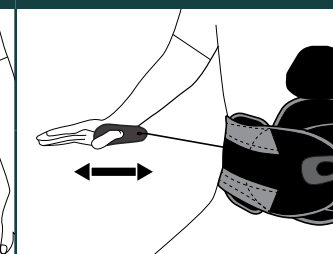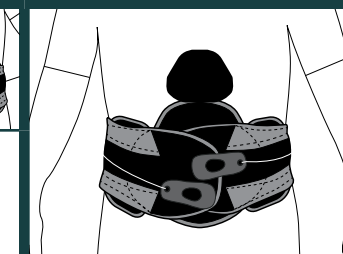

5. ADJUSTMENT

A. Adjust the upper and/or lower compression by loosening or tightening the pull tabs as needed.
B. When patient is seated, slightly loosening the upper portion may be beneficial.